

Electrocardiogram (ECG) RBRCLA_ECG_001

Purpose

To provide a high throughput method to obtain Electrocardiograms in a conscious mouse.

Experimental Design

- **Minimum number of animals** : 5M + 5F
- **Age at test**: Week 52
- **Sex**: We would expect the results of this test to show sexual dimorphism

Procedure

1. The lead plates are to be snapped into place onto the top of the pre-amplifier tower. The covering is removed to reveal three gel coated pads surrounded by a sticking plate. The plate will need to be covered with the extra cover in the package.
2. Turn on the combined amplifier and the pre-amplifier tower.
3. Double click the icon ECG acquisition on the acquisition computer.
4. Open the ECG set up file (for default settings).
6. Place mouse on pad, lowering the Red Acrylic Cubby to surround the mouse on 3 sides discouraging escape.
7. Press Start.
8. After the desired acquisition time, (5-10 minutes) stop the reading. There will be one long reading.
9. Save the data.
10. For additional readings create a new session using the same settings as before.
11. When saving sections with good readings, highlight the selected area and then save.



Notes

Data Analysis

1. Open Emouse Analyses icon
2. Select ECG signals
3. Choose folder (all readings in folder will show)
4. Click PNN X (for mice: N-N> than 6 ms)
5. Choose file(s) by highlighting
6. Go
7. Bottom file is the corrected file
8. Red dots should be on peak of R waves, if image appears inverted click invert
9. Click Add, or minus if R waves are not marked with red dots or if too many are marked
 - L click to zoom in

- R click to zoom out
10. 'What if?' button to remove unwanted sections
 - L click image (zooms in)
 - L click left boundary
 - L click right boundary
 11. Options- click more if want to exclude more sections
 12. Undo available
 13. Go
 14. Here can input animal data if desired
 15. Save- For the first mouse in in group, hit save, a new results folder will be created within the folder with the mouse data. Then can click quick save or next.
 16. For the rest of the mice in the series, can hit quick save at this point- saves in last selected file – will group all files together in same excel sheet.
 17. Open Emouse Analyses icon
 18. Select ECG signals
 19. Choose folder (all readings in folder will show)
 20. Click PNN X (for mice: N-N> than 6 ms)
 21. Choose file(s) by highlighting
 22. Go
 23. Bottom file is the corrected file
 24. Red dots should be on peak of R waves, if image appears inverted click invert
 25. Click Add, or minus if R waves are not marked with red dots or if too many are marked
 - L click to zoom in
 - R click to zoom out
 26. 'What if?' button to remove unwanted sections
 - L click image (zooms in)
 - L click left boundary
 - L click right boundary
 27. Options- click more if want to exclude more sections
 28. Undo available
 29. Go
 30. Here can input animal data if desired
 31. Save- For the first mouse in in group, hit save, a new results folder will be created within the folder with the mouse data. Then can click quick save or next
 32. For the rest of the mice in the series, can hit quick save at this point- saves in last selected file - will group all files together in same excel sheet

Examples of good readings

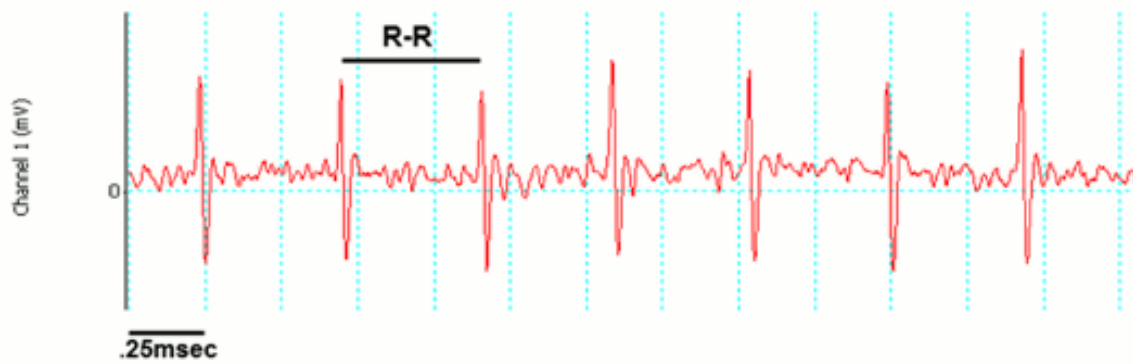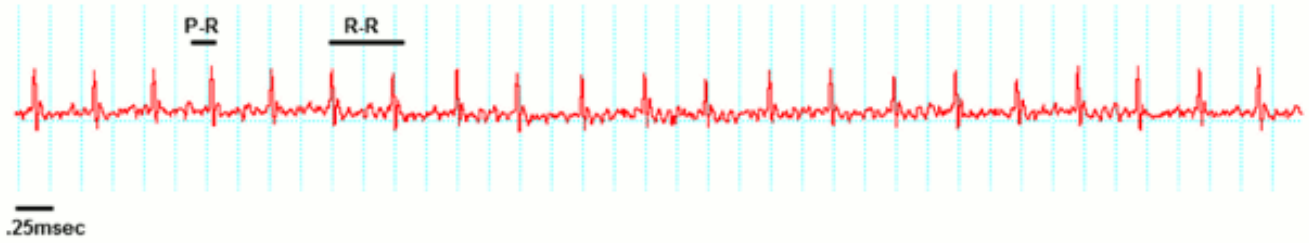A**B**

Data QC

Analysis room should be dim and quiet. Keep the door closed preferably while analysis is taking place.

Figure A. Taking a reading

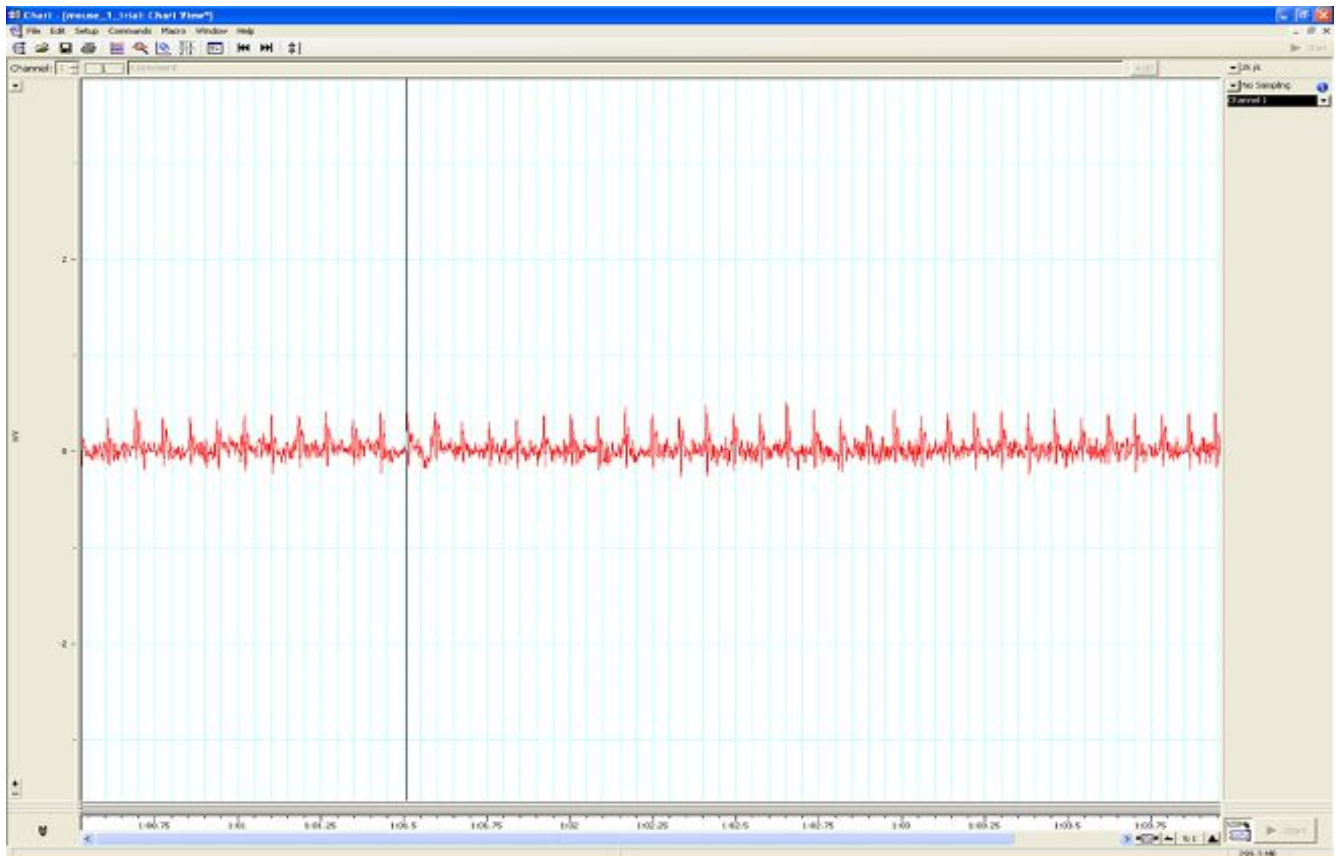


Figure B. Saving a section of the reading


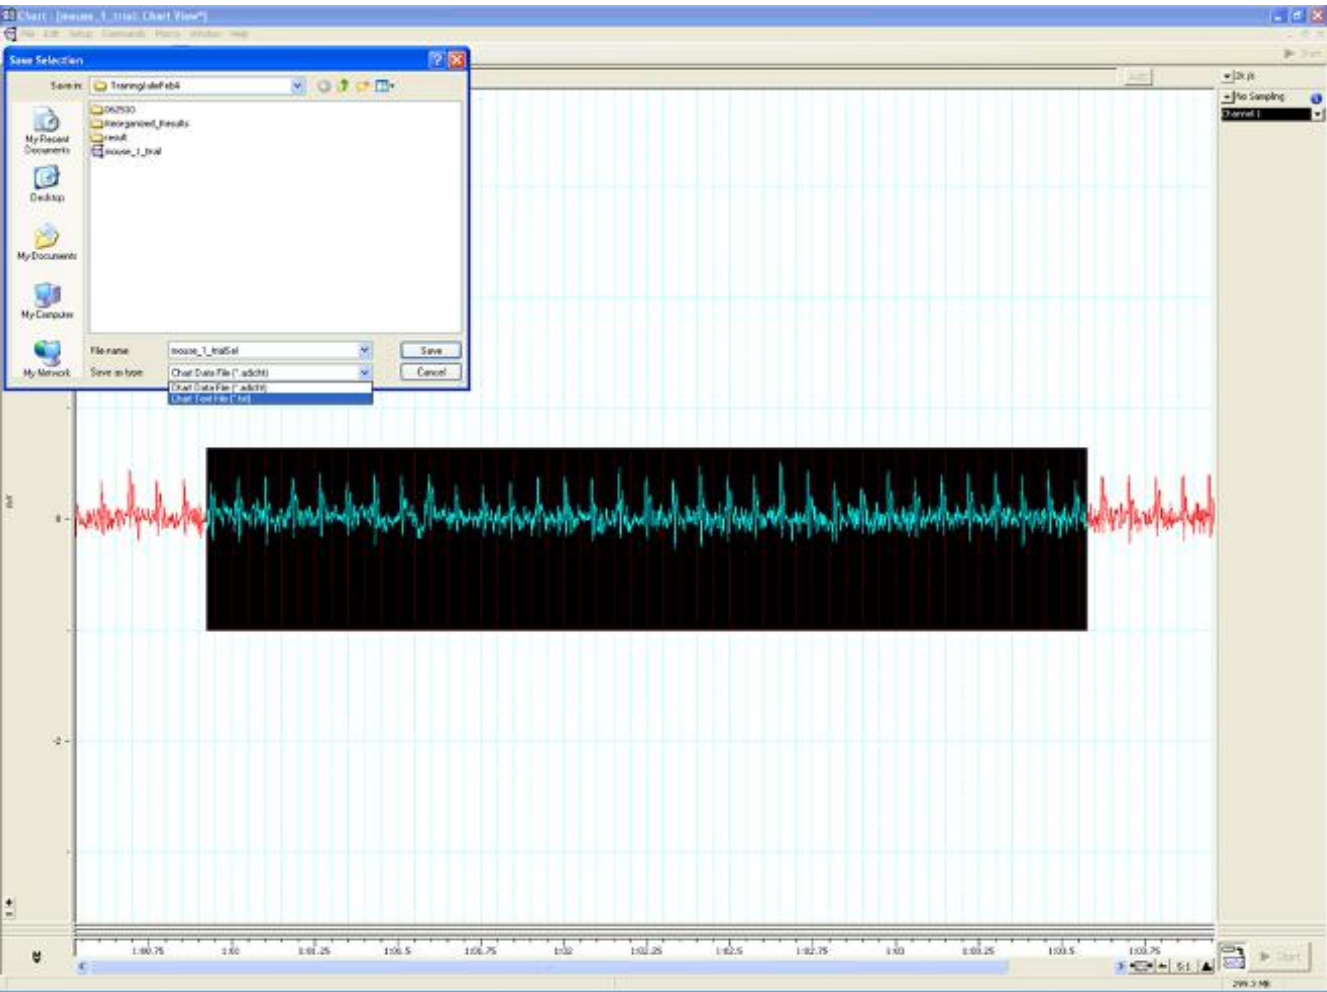


Figure C. Analysis phase, with the options to remove sections on the 'What if?' button below.

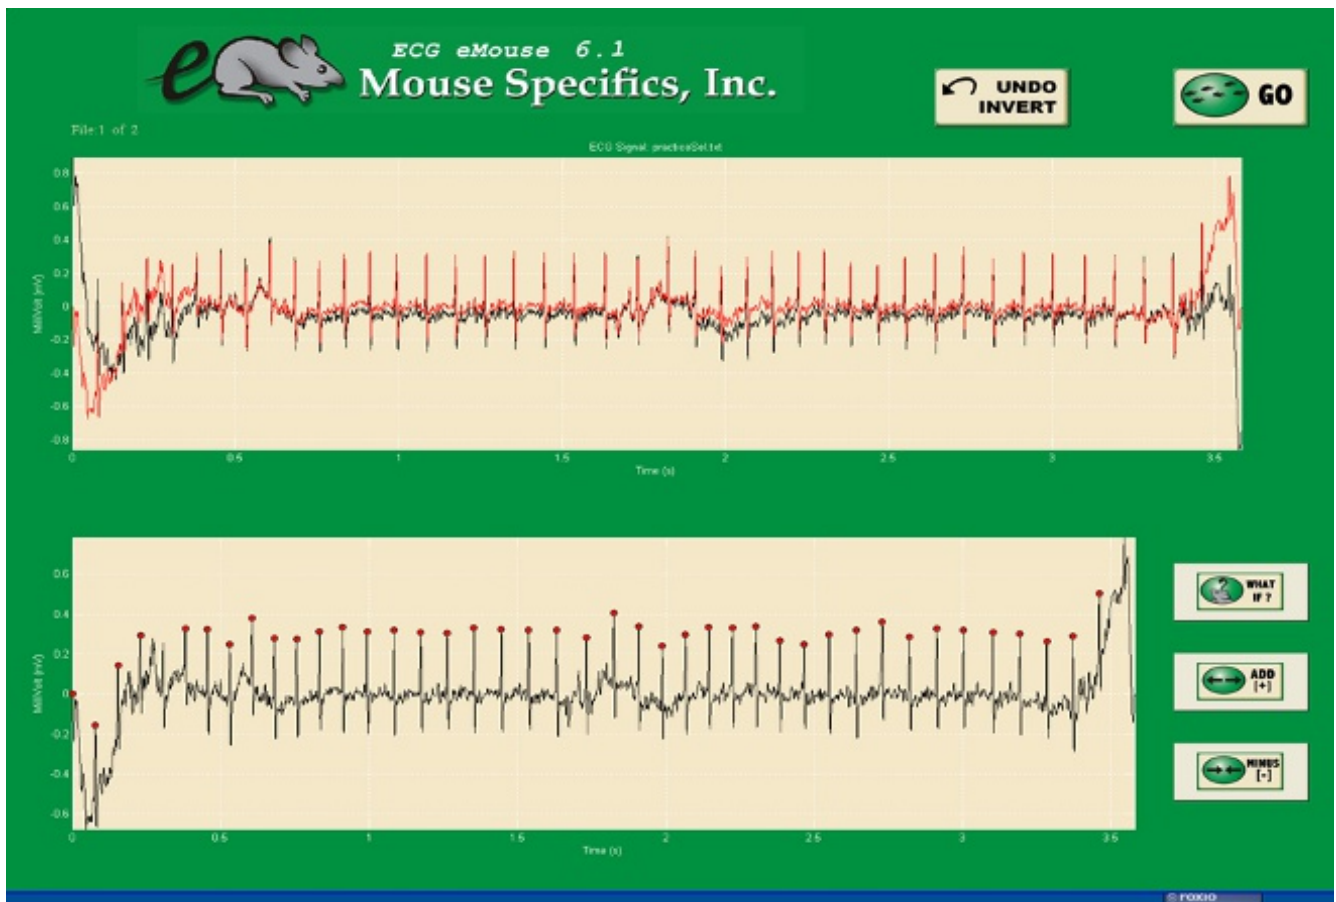

Parameters and Metadata

Number of signals RBRCLA_ECG_001_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: true

Is Annotated: false

HR RBRCLA_ECG_002_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: true

Is Annotated: true

Unit Measured: bpm

CV RBRCLA_ECG_003_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: false

Is Annotated: true

Unit Measured: %

RR RBRCLA_ECG_004_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: true

Is Annotated: true

Unit Measured: ms

PQ RBRCLA_ECG_005_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: false

Is Annotated: true

Unit Measured: ms

PR RBRCLA_ECG_006_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: true

Is Annotated: true

Unit Measured: ms

QRS RBRCLA_ECG_007_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: true

Is Annotated: true

Unit Measured: ms

ST RBRCLA_ECG_008_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: true

Is Annotated: true

Unit Measured: ms

QTc RBRCLA_ECG_009_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: true

Is Annotated: false

Unit Measured: ms

HRV RBRCLA_ECG_010_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: false

Is Annotated: true

Unit Measured: bpm

QTc Dispersion RBRCLA_ECG_011_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: false

Is Annotated: false

Unit Measured: ms

Mean SR amplitude RBRCLA_ECG_012_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: false

Is Annotated: false

Unit Measured: mV

Mean R amplitude RBRCLA_ECG_013_001 | v1.0

simpleParameter

Req. Analysis: false Req. Upload: false Is Annotated: false

Unit Measured: mV

rMSSD RBRCLA_ECG_014_001 | v1.0

simpleParameter

Req. Analysis: false Req. Upload: false Is Annotated: true

Unit Measured: ms

pNN5(6>ms) RBRCLA_ECG_015_001 | v1.0

simpleParameter

Req. Analysis: false Req. Upload: false Is Annotated: false

Unit Measured: %

Equipment ID RBRCLA_ECG_016_001 | v1.0

procedureMetadata

Req. Analysis: false

Req. Upload: true

Is Annotated: false

Equipment Manufacturer RBRCLA_ECG_017_001 | v1.0

procedureMetadata

Req. Analysis: true

Req. Upload: true

Is Annotated: false

Options: Mouse Specifics, Inc., AD Instruments, World Precision Instruments,

Equipment Model RBRCLA_ECG_018_001 | v1.0

procedureMetadata

Req. Analysis: true

Req. Upload: true

Is Annotated: false

Options: ECGenie, ML870/p, ML826/FE132, Iso-DAM8A, ECGenie + gel pads, ML866, PowerLab: 4/35,

Anesthetic RBRCLA_ECG_019_001 | v1.0

procedureMetadata

Req. Analysis: true

Req. Upload: true

Is Annotated: false

Options: Isoflurane, Avertin, Tribromoethanol, No anesthesia,

Experimenter ID RBRCLA_ECG_020_001 | v1.0

procedureMetadata

Req. Analysis: false

Req. Upload: true

Is Annotated: false

Noise level RBRCLA_ECG_021_001 | v1.0

procedureMetadata

Req. Analysis: false

Req. Upload: false

Is Annotated: false

Light level RBRCLA_ECG_022_001 | v1.0

procedureMetadata

Req. Analysis: false

Req. Upload: false

Is Annotated: false

Date equipment last calibrated RBRCLA_ECG_023_001 | v1.0

procedureMetadata

Req. Analysis: false

Req. Upload: false

Is Annotated: false

Analysis Software RBRCLA_ECG_024_001 | v1.0

procedureMetadata

Req. Analysis: true

Req. Upload: false

Is Annotated: false

Options: eMouse, Matlab,

Waveform Image RBRCLA_ECG_025_001 | v1.0

seriesMediaParameter

Req. Analysis: false

Req. Upload: false

Is Annotated: false

Increments: Minimum 1

Waveform Image Comment RBRCLA_ECG_026_001 | v1.0

simpleParameter

Req. Analysis: false

Req. Upload: false

Is Annotated: false

Description:

Free text comment on the waveform image. Use parameterAssociation of the image parameter to link to this text.
